



5-Blue 6-Violet 2-355UV 3-Red Trop Bien


Cytometer:	LSRII	User:	BDService
Cytometer Name:	LSRII	Institution:	
Serial Number:	1	Software:	BD FACSDiva 6.1.2
Input Device:	Manual	Date:	8/3/2016 12:18:14 PM
Window Extension:	10.00		

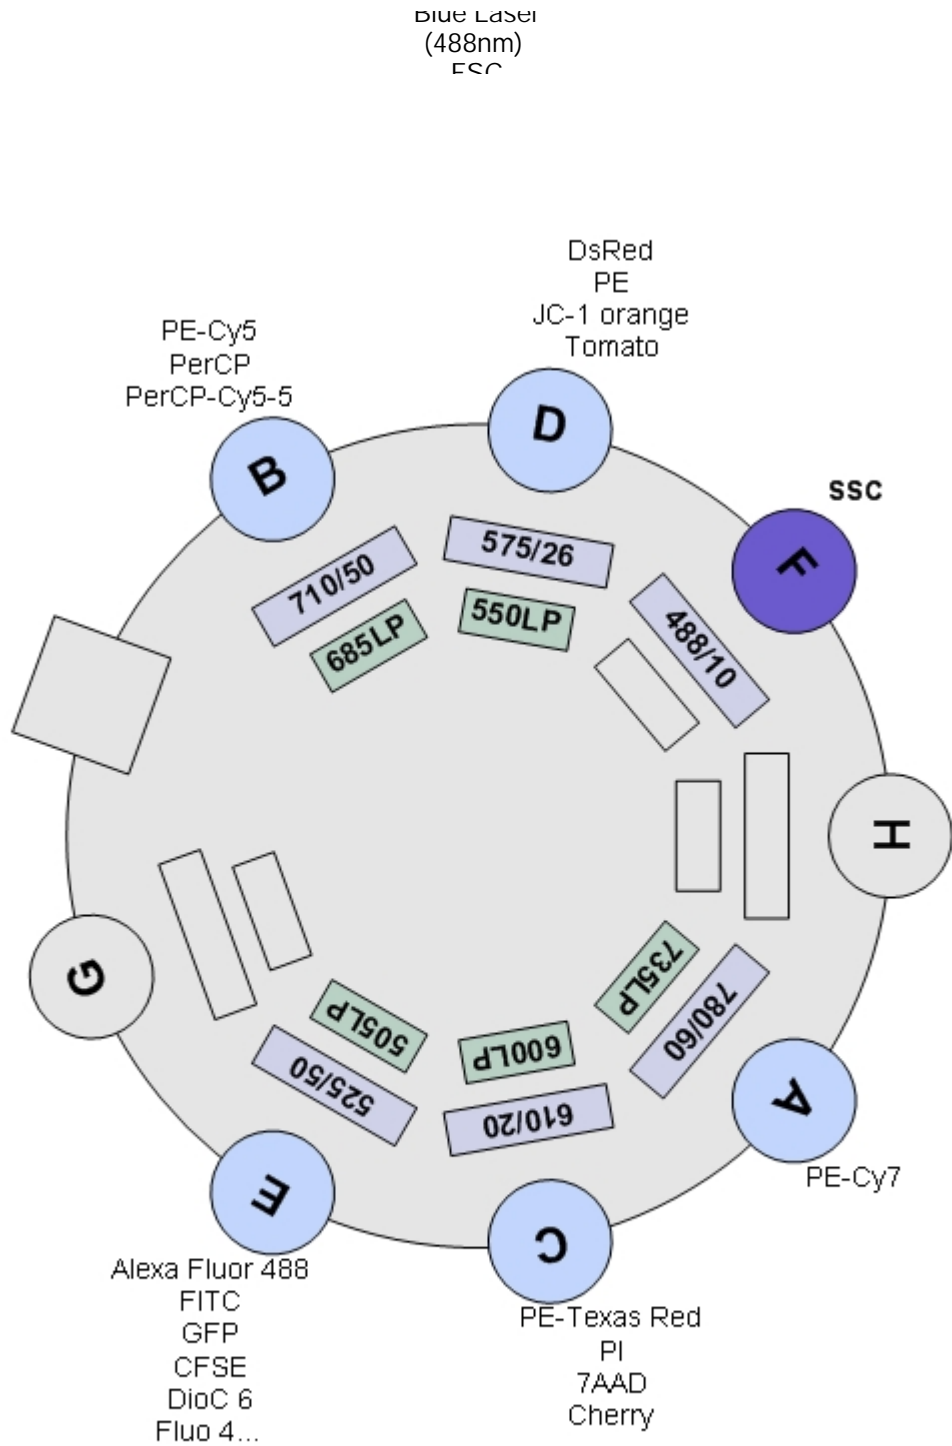


Violet Laser
(405nm)

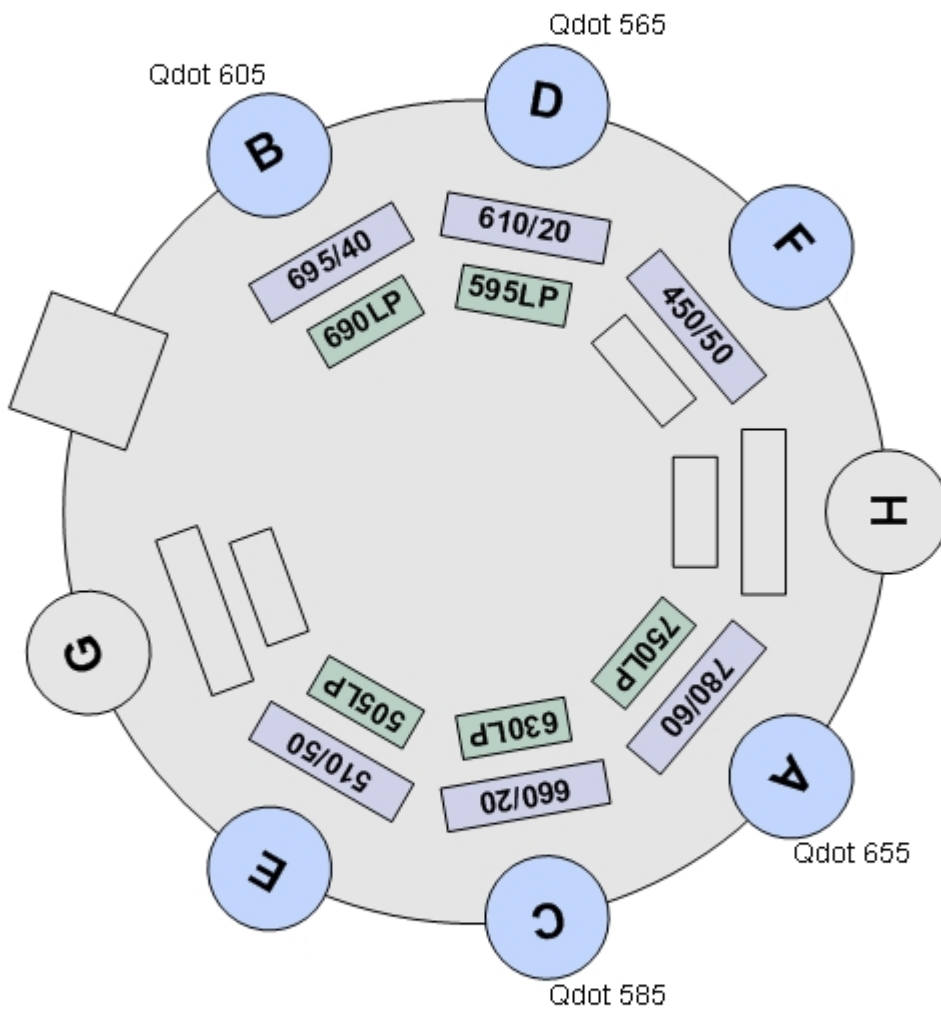

355 UV Laser
(355nm)

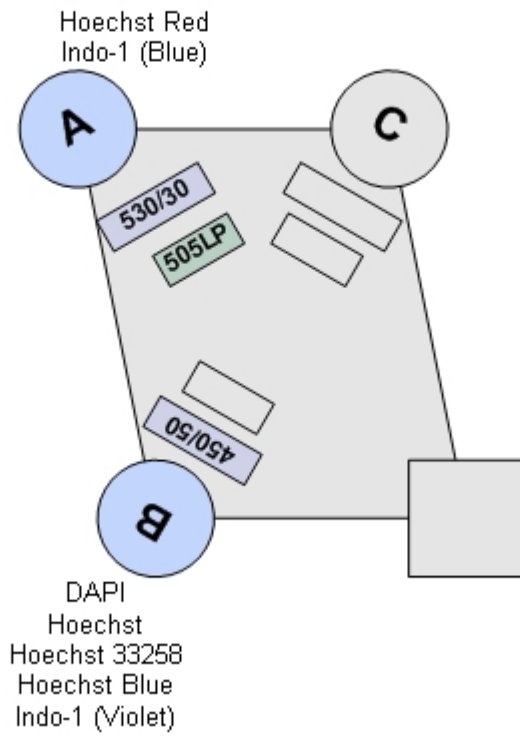

Red Laser
(633nm)

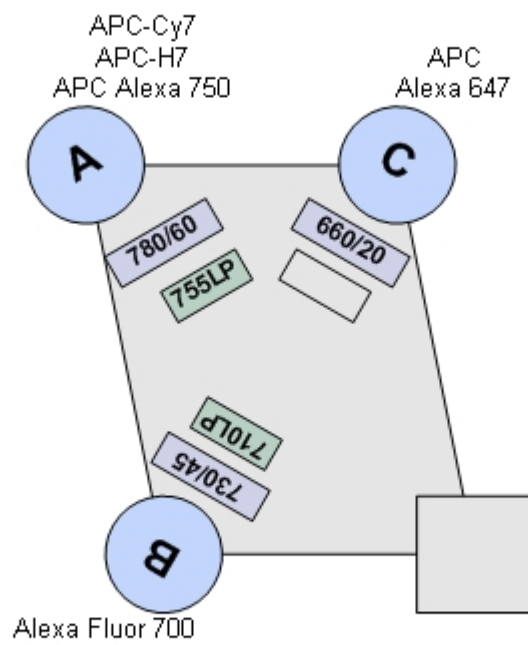

Comments: