



Aria III100u 20 Psi 488, 561, 633, 405 (3-5-3-6)

Cytometer:	FACSAriaIII	User:	Administrator
Cytometer Name:	FACSAriaIII	Institution:	N/A
Serial Number:	1	Software:	BD FACSDiva 8.0.1
Input Device:	Manual	Date:	8/3/2016 12:08:18 PM
Sheath Pressure:	20.00		
Nozzle Size:	100		
Window Extension:	2.00		


Blue Laser
(488nm)
FSC

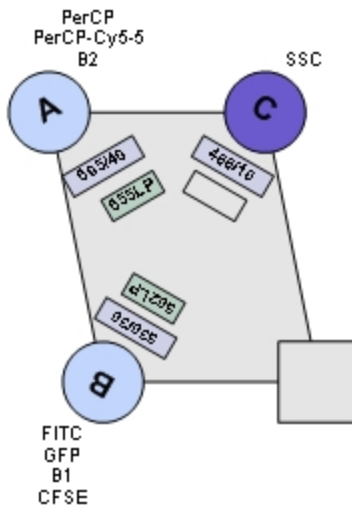


561 Yellow-Green Laser
(561nm)

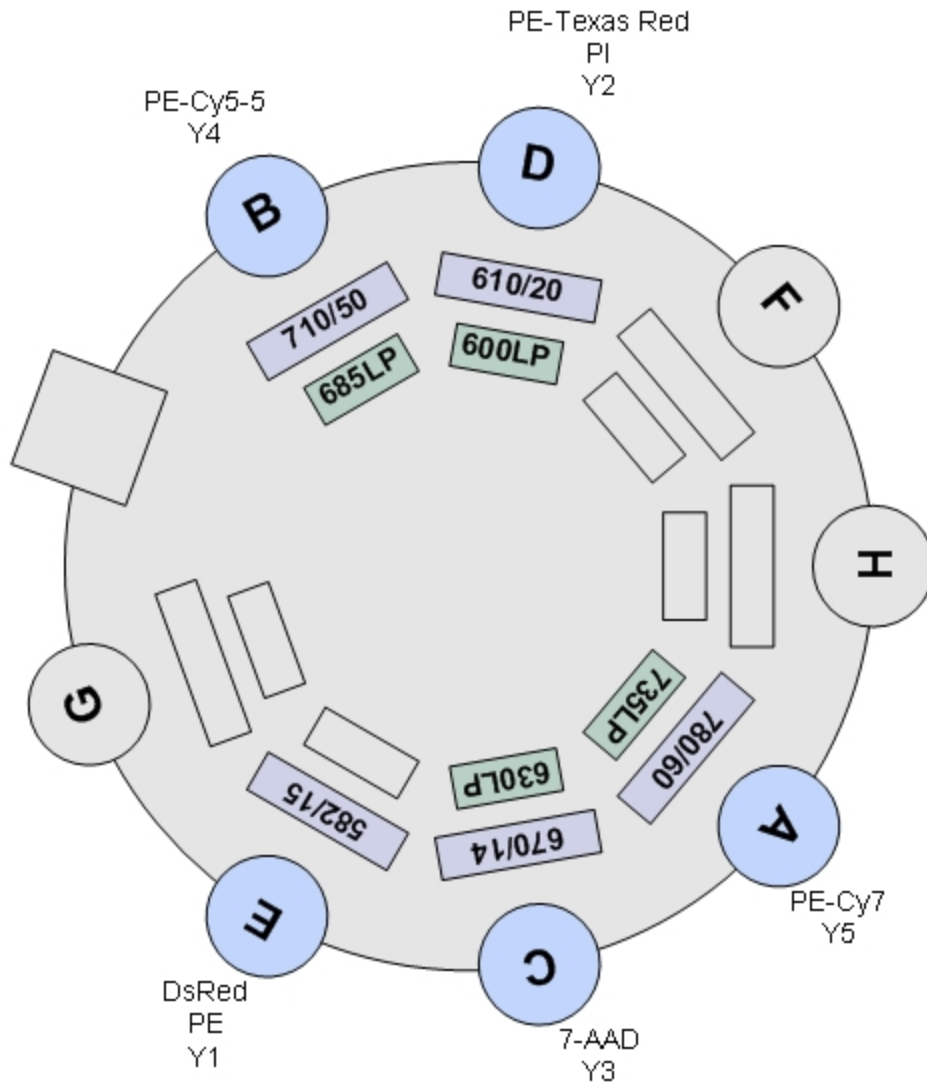

Red Laser
(633nm)

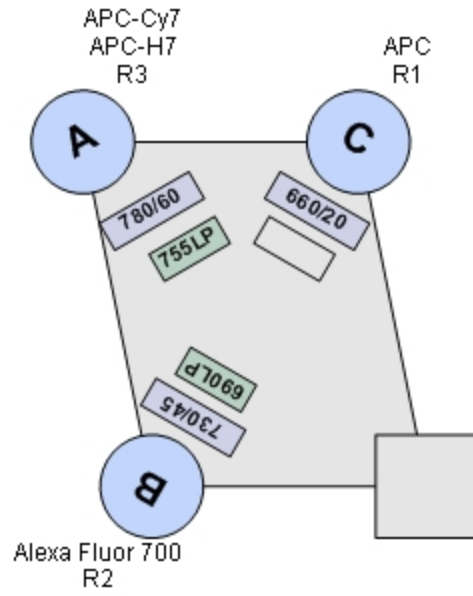

Violet Laser
(405nm)

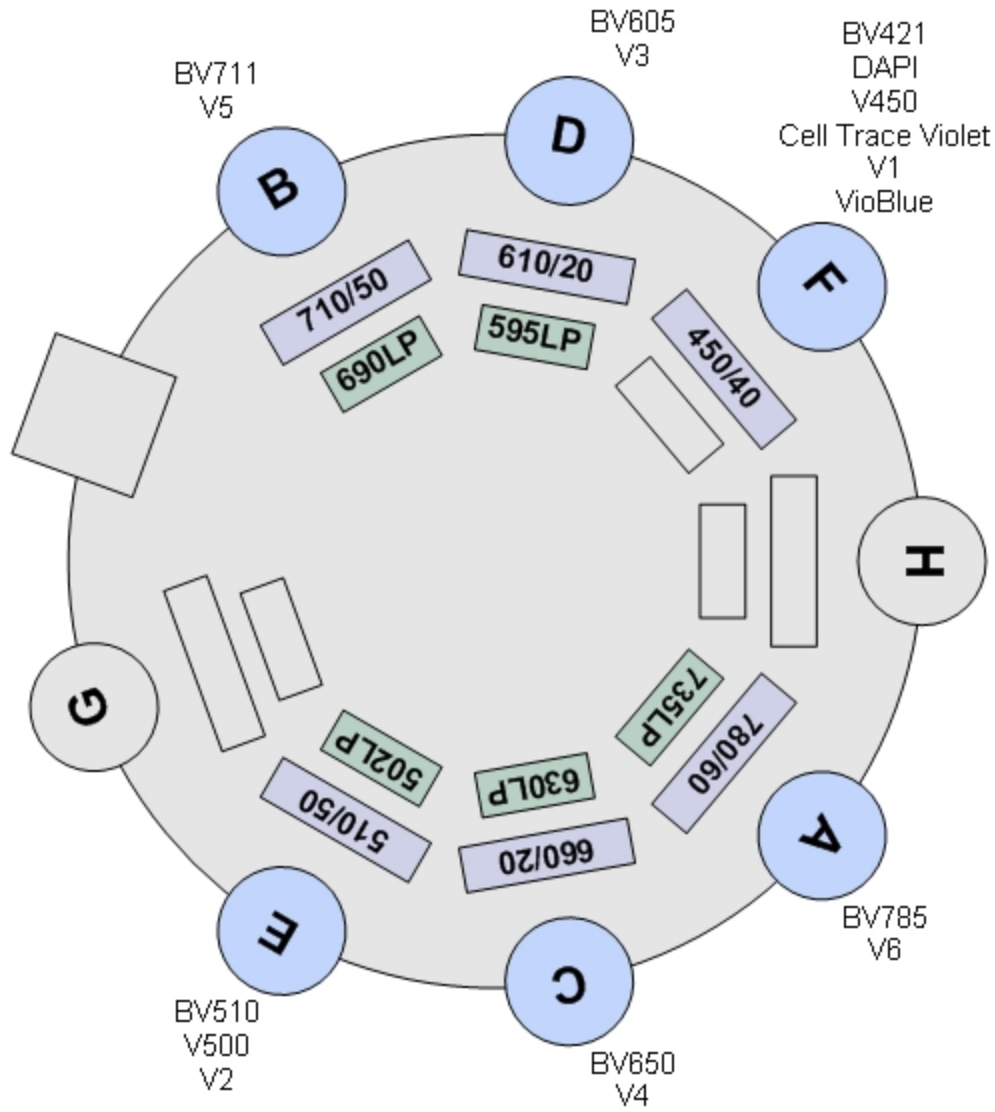

Comments: